

SAFETY OF BLOOD PRODUCTS

THERAFLEX UV Platelets

PATHOGEN INACTIVATION SYSTEM FOR PLATELET CONCENTRATES


MacoPharma's latest development in the Safety of Blood Product Range:

- No photosensitizer
- Two step process
- 60 second UVC irradiation

Performance Targets:

- Apheresis and Buffy-coat derived platelet concentrates
- Efficacy on Bacteria, Spores, Non-envelopped and Envelopped Viruses, Leucocytes, Parasites
- Storage up to 7 days with SSP+

THERAFLEX UV Platelets: 2 step process

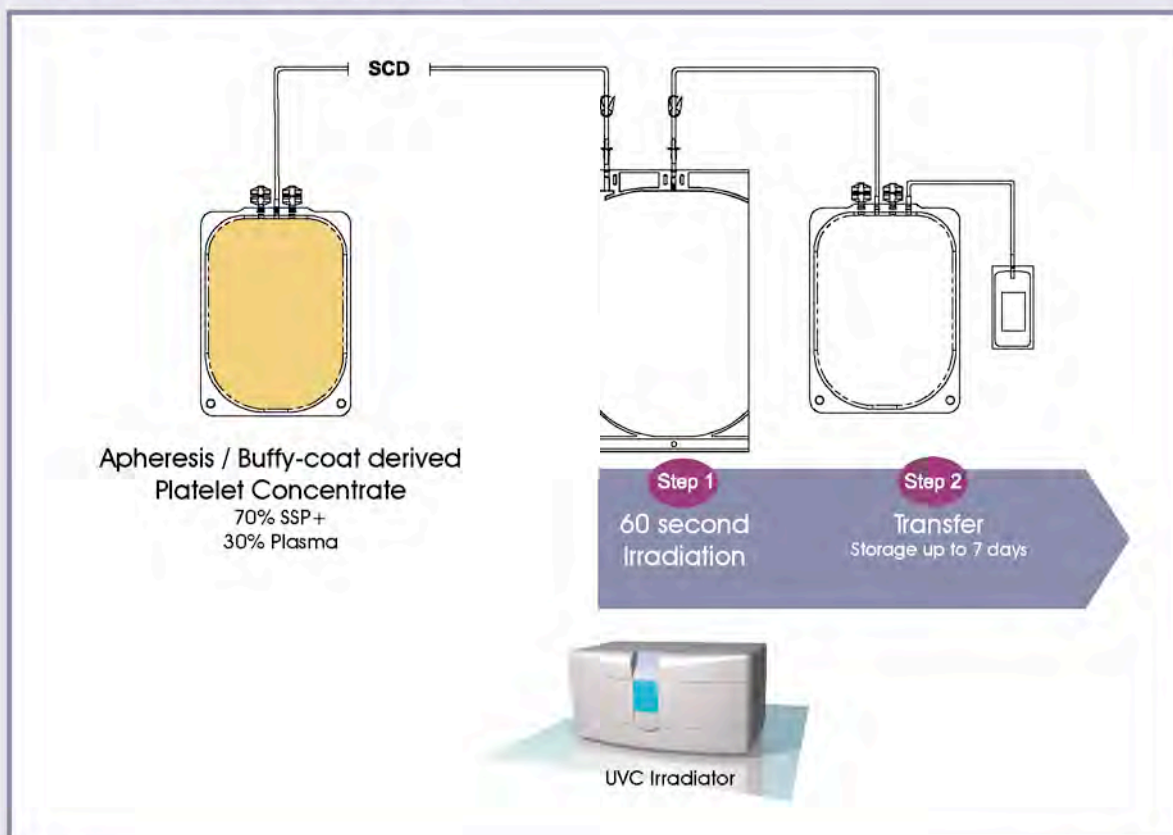

A NOVEL TECHNIQUE FOR PATHOGEN INACTIVATION AND ITS EFFECT ON THE QUALITY OF PLATELET CONCENTRATES: THERAFLEX UV PLATELETS

Walker W H¹, Tolksdorf F¹, Mohr H², Gravemann U², Müller T H²,

¹ MacoPharma International GmbH, Langen, Germany

² German Red Cross Chapters of NSTOB, Springe, Germany

ISBT Regional Congress Asia, Hanoi, November 2007

INTRODUCTION

The use of a pathogen inactivation technology is an option to enhance the safety of platelet transfusions. Current procedures need chemicals to be added to the platelet concentrates (PCs). These compounds are of concern if they remain in the final product. Moreover, treatment may cause deterioration of the platelets. A novel procedure has been developed using only short-wave UV light (UVC, 254 nm) that effectively inactivates pathogens in plasma-reduced PCs. The equipment used consists of an irradiation device with a specific mechanism for agitation. Its capacity is one platelet unit (random donor or apheresis) per treatment cycle. Treatment parameters, e.g. UVC intensity, UVC dose, temperature and agitation, are microprocessor-controlled. Platelets are processed in the THERAFLEX twin-bag kit, which comprises a highly UV-transparent polyolefin acetate bag[1] for irradiation and a platelet storage container (Fig.1, 2). It was investigated to what extent platelet integrity and storage stability of the treated products were influenced by this new inactivation procedure.

MATERIALS & METHODS

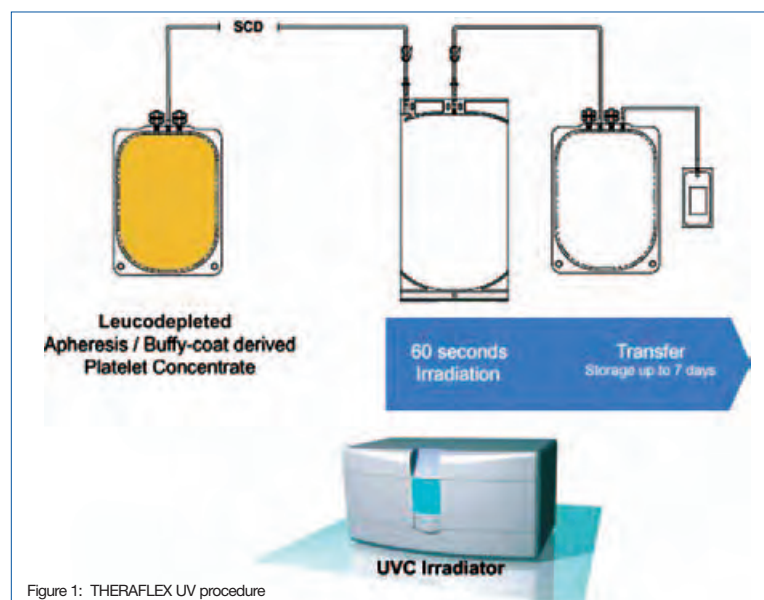


Figure 1: THERAFLEX UV procedure

Plasma-reduced PCs were treated with the THERAFLEX UV procedure (Fig.1) and stored until day 8 after blood donation (day 6 after treatment). The in vitro quality of UVC treated PCs was evaluated in comparison to non-treated control platelets. Control PCs were stored for the same time period. PCs in storage medium SSP+ (MacoPharma) were prepared from pools of 5 buffy coats. The average volume treated was 350 mL. Plasma concentration was approx. 30%. PCs were transferred into irradiation bags (Fig.2) and treated with UVC light at a dose of 0.4 J/cm² (approx. 60 sec) (Fig.3). They were strongly agitated during irradiation.



Figure 2: Twin-bag kit

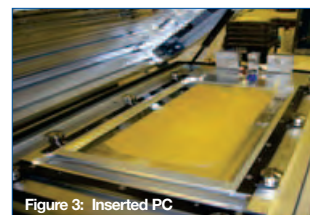


Figure 3: Inserted PC

RESULTS

In vitro characteristics were hardly influenced by the THERAFLEX treatment. HSR reactivity was only slightly reduced whereas collagen induced aggregation was moderately increased. Glucose consumption and lactate formation were found to be marginally higher in the treated PCs. Thus, pH slightly dropped but remained above 7.0 until day 8 after donation. The mean platelet loss due to UVC treatment was 4% (Tab.1).

Day 3	Plts [x10 ⁹ /mL]	HSR [%]	pH	Spontaneous aggregation [%]	Collagen-ind. aggregation 100 µg/mL [%]	Glucose [mg/dL]	Lactate [mmol/L]
Control	10.2 ± 1.6	68 ± 4	7.13 ± 0.05	11 ± 3	94 ± 3	122 ± 8	7.5 ± 1.0
Treated	9.6 ± 1.3	64 ± 5	7.07 ± 0.07	14 ± 2	89 ± 5	118 ± 6	7.7 ± 0.8
Day 6							
Control	9.9 ± 1.0	66 ± 2	7.24 ± 0.13	12 ± 2	74 ± 9	86 ± 10	10.8 ± 1.0
Treated	9.5 ± 1.3	64 ± 8	7.09 ± 0.06	14 ± 3	81 ± 9	68 ± 10	12.8 ± 1.5
Day 8							
Control	9.4 ± 1.6	68 ± 1	7.29 ± 0.12	10 ± 1	62 ± 7	63 ± 9	12.5 ± 0.9
Treated	9.1 ± 1.3	61 ± 8	7.09 ± 0.05	16 ± 4	69 ± 7	41 ± 8	15.2 ± 1.0

Table 1: Platelet parameters of untreated and treated PCs on day 3, 6 and 8 after blood donation (mean ± SD; n=4)

CONCLUSIONS

Plasma-reduced PCs were only slightly affected when treated with the THERAFLEX UV system for pathogen inactivation. In vitro parameters and storage stability were well preserved until day 8 after blood donation.

[1] Polyolefineacetate bags for pathogen inactivation and for storage of platelet concentrates, H Mohr, TH Müller, F Tolksdorf, WH Walker, Vox Sang 2004; 87 (Suppl. 3): 70

PATHOGEN REDUCTION IN PLATELET CONCENTRATES USING UVC LIGHT IN COMBINATION WITH STRONG AGITATION: EFFECT ON ACTIVATION MARKERS AND STORAGE STABILITY

Tolksdorf F¹, Walker W H¹, Mohr H², Gravemann U², Mueller T H²


¹ Maco Pharma, Langen, Germany, ² Blood Centre of German Red Cross Chapters of NSTOB, Institute Springe, Germany

AABB Annual Meeting 2007, Anaheim, USA


INTRODUCTION

Pathogen Inactivation technologies are proactive measures to enhance the safety of platelet transfusions. Their use can be effective also against emerging unknown pathogens. Current procedures need chemicals like photosensitizers. We developed a procedure, which allows an efficient reduction of pathogens (e.g. bacteria and viruses) in plasma-reduced platelet concentrates (PCs) using short-wavelength UV light (UVC) in combination with strong agitation, i.e. there is no photoactive compound needed (THERAFLEX UV Platelets technology). The irradiation device developed is emitting UVC light at a wavelength of 254 nm. Moreover a mechanism for orbital agitation is installed. UVC irradiation is microprocessor-controlled. Relevant treatment parameters are monitored throughout the entire treatment thus allowing a fully documented and reproducible process. PCs are treated in a twin-bag kit, which comprises of a highly UV-permeable irradiation bag and a container for extended platelet storage. In the present study we investigated the influence of the THERAFLEX UV treatment on activation parameters and on the storage stability of PCs.

MATERIALS & METHODS

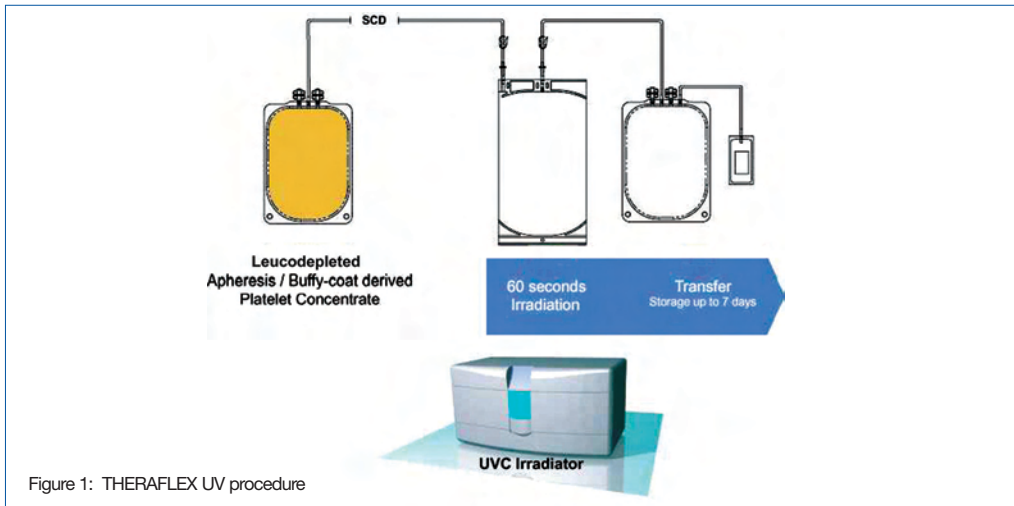

Plasma-reduced PCs were treated with the THERAFLEX UV procedure (Fig.1) and stored until day 8 after blood donation (day 6 after treatment). The in vitro quality of UVC treated PCs was evaluated in comparison to untreated control platelets. Control PCs were stored for the same time period. PCs in storage medium SSP+/MacoPharma (containing saline, citrate, acetate, phosphate, magnesium and potassium, identical to PAS-IIIM) were prepared from pools of 5 buffy coats. The average volume was 350 mL (platelet concentration approx. 10^9 /mL) and the plasma concentration was approx. 35%. PCs were transferred into irradiation bags (Fig.2) for UVC treatment at a dose of 0.4 J/cm^2 (approx. 60 sec) (Fig.3). They were strongly agitated during irradiation. Relevant treatment parameters, e.g. UV dose, UV intensity, temperature and irradiation time, were microprocessor-controlled.

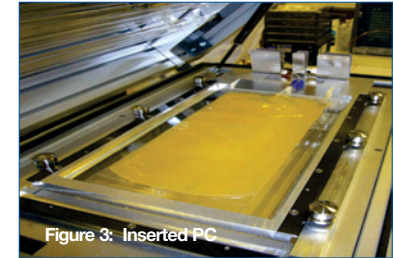

RESULTS

Until day 8 of storage in vitro characteristics were only marginally influenced by the THERAFLEX process. Platelet quality was evaluated by measurement of the hypotonic shock response (HSR) and the expression of the activation marker CD62p. HSR reactivity and CD62p levels were only slightly affected by the Theraflex treatment. Annexin V binding percentage, as a marker for apoptosis, remained almost unchanged. Glucose consumption and lactate formation were found to be marginally higher in the treated PCs. pH remained above 7.0 until day 8 after donation (Tab. 1).

	Pits [$\times 10^9$ /mL]	CD62 [%]	Annexin V [%]	HSR [%]	pH	Glucose [mg/dL]	Lactate [mmol/L]
Day 6*							
Control	9.2 ± 1.1	21 ± 6	5 ± 1	71 ± 5	7.29 ± 0.04	62 ± 17	10.2 ± 2.3
Treated	8.5 ± 0.9	32 ± 5	9 ± 4	68 ± 4	7.22 ± 0.05	52 ± 21	10.8 ± 1.6
Day 7*							
Control	8.9 ± 0.8	24 ± 6	7 ± 1	72 ± 3	7.32 ± 0.05	55 ± 19	10.4 ± 1.6
Treated	8.4 ± 0.9	42 ± 13	10 ± 3	68 ± 3	7.22 ± 0.06	42 ± 20	11.8 ± 1.7
Day 8*							
Control	9.4 ± 1.6	30 ± 3	8 ± 4	71 ± 5	7.34 ± 0.06	45 ± 18	11.5 ± 1.6
Treated	9.1 ± 1.3	52 ± 12	10 ± 3	65 ± 5	7.22 ± 0.09	31 ± 17	13.1 ± 1.7

Table 1: In vitro parameters of untreated and treated PCs on day 6, 7 and 8 after blood donation (N = 6, mean \pm SD)

*after blood donation

CONCLUSIONS

THERAFLEX treatment with 0.4 J/cm^2 UVC light has only a minor influence on in vitro parameters of PCs and their storage stability until day 8 after blood donation was maintained.

[1] Polyolefineacetate bags for pathogen inactivation and for storage of platelet concentrates, H Mohr, TH Müller, F Tolksdorf, WH Walker, Vox Sang 2004; 87 (Suppl. 3): 70

Funded by Forschungsgemeinschaft der Blutspendendienste des Deutschen Roten Kreuzes e.V. and Maco Pharma.

IN VITRO QUALITY AND STORAGE STABILITY OF PLATELET CONCENTRATES AFTER THERAFLEX UV TREATMENT

Tolksdorf F¹, Walker W H¹, Mohr H², Gravemann U², Müller T H²

¹MacoPharma, Langen, Germany

²Blood Centre of the German Red Cross Chapters of NSTOB, Institute Springe, Germany

DGTI Congress, Friedrichshafen, September 2007

INTRODUCTION

Pathogen Inactivation technologies are proactive measures to enhance the safety of platelet transfusions. Their use can be effective also against emerging unknown pathogens. Current procedures need chemicals like photosensitizers. We developed a procedure, which allows an efficient reduction of pathogens (e.g. bacteria and viruses) in plasma-reduced platelet concentrates (PCs) using short-wavelength UV light (UVC) in combination with strong agitation, i.e. there is no photoactive compound needed (THERAFLEX UV Platelets technology). The irradiation device developed for this purpose is equipped with a light source emitting UVC light at a wavelength of 254 nm. Moreover a mechanism for orbital agitation is installed. UVC irradiation is microprocessor-controlled. Relevant treatment parameters are monitored throughout the entire treatment thus allowing a well documented and reproducible process. PCs are treated in a twin-bag kit, which comprises of a highly UV-permeable irradiation bag and a container for extended platelet storage. In the present study we investigated the influence of the THERAFLEX UV treatment on in vitro parameters of PCs and on their storage stability.

MATERIALS & METHODS

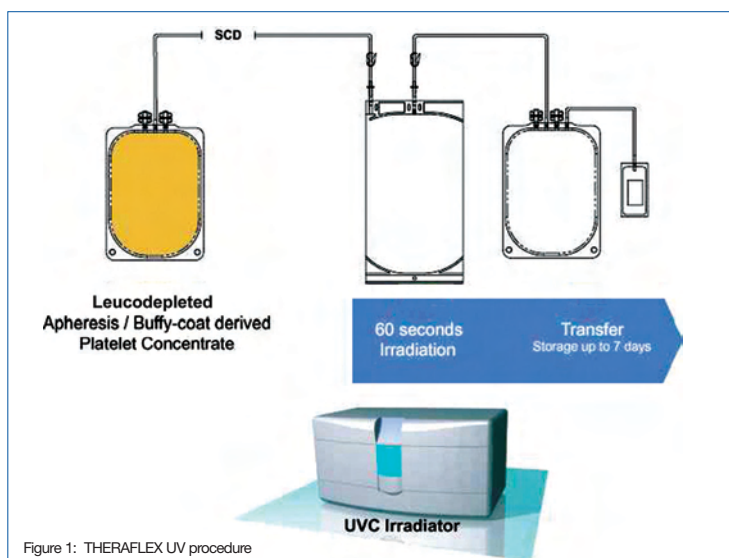


Figure 1: THERAFLEX UV procedure

Plasma-reduced PCs were treated with the THERAFLEX UV procedure (Fig.1) and stored until day 8 after blood donation (day 6 after treatment). The in vitro quality of UVC treated PCs was evaluated in comparison to untreated control platelets. Control PCs were stored for the same time period. PCs in storage medium SSP+ (containing saline, citrate, acetate, phosphate, magnesium and potassium, identical to PAS-IIIM) were prepared from pools of 5 buffy coats. The average volume was 350 mL and the plasma concentration was approx. 35%. PCs were transferred into irradiation bags (Fig.2) for UVC treatment. After insertion into the irradiation device (Fig.3) PCs were treated with UVC light at a dose of 0.4 J/cm² (approx. 60 sec). They were strongly agitated during irradiation. The system was microprocessor-controlled. The control unit enables monitoring and recording of relevant treatment parameters like UV dose, UV intensity, temperature and irradiation time.



Figure 2: Twin-bag kit




Figure 3: Inserted PC

RESULTS

Until day 8 of storage in vitro characteristics were only marginally influenced by the THERAFLEX process. Platelet activation was evaluated by measurement of the hypotonic shock response (HSR) and the expression of the activation marker CD62p. HSR was only slightly and CD62p levels were moderately affected by Theraflex treatment. Annexin V binding percentage, as a marker for apoptosis, remained almost unchanged. Glucose consumption and lactate formation were found to be marginally higher in the treated PCs. pH remained above 7.0 until day 8 after donation (Tab. 1).

Day 6*	Plts [x10 ⁹ /mL]	HSR [%]	pH	CD62 [%]	Annexin V [%]	Glucose [mg/dL]	Lactate [mmol/L]
Control	9.2 ± 1.1	71 ± 5	7.29 ± 0.04	21 ± 6	5 ± 1	62 ± 17	10.2 ± 2.3
Treated	8.5 ± 0.9	68 ± 4	7.22 ± 0.05	32 ± 5	9 ± 4	52 ± 21	10.8 ± 1.6
Day 7*							
Control	8.9 ± 0.8	72 ± 3	7.32 ± 0.05	24 ± 6	7 ± 1	55 ± 19	10.4 ± 1.6
Treated	8.4 ± 0.9	68 ± 3	7.22 ± 0.06	42 ± 13	10 ± 3	42 ± 20	11.8 ± 1.7
Day 8*							
Control	9.4 ± 1.6	71 ± 5	7.34 ± 0.06	30 ± 3	8 ± 4	45 ± 18	11.5 ± 1.6
Treated	9.1 ± 1.3	65 ± 5	7.22 ± 0.09	52 ± 12	10 ± 3	31 ± 17	13.1 ± 1.7

Table 1: In vitro parameters of untreated and treated PCs on day 6, 7 and 8 after blood donation (N=6, mean ± SD)

*after blood donation

CONCLUSIONS

THERAFLEX treatment with 0.4 J/cm² UVC light has only a minor influence on in vitro parameters of PCs and on their storage stability until day 8 after blood donation.

Funded by Forschungsgemeinschaft der Blutspendedienste des Deutschen Roten Kreuzes e.V. and Maco Pharma.

THERAFLEX UV PLATELETS: A NOVEL TECHNIQUE FOR PATHOGEN INACTIVATION AND ITS EFFECT ON THE QUALITY OF PLATELET CONCENTRATES

Tolksdorf F¹, Walker W H¹, Mohr H², Gravemann U², Müller T H²

¹MacoPharma, Langen, Germany


²Blood Centre of the German Red Cross Chapters of NSTOB, Institute Springe, Germany

ISBT Congress, Madrid, June 2007

INTRODUCTION

The use of a pathogen inactivation technology is an option to enhance the safety of platelet transfusions. Current procedures need chemicals to be added to the platelet concentrates (PCs). These compounds are of concern if they remain in the final product. Moreover, treatment may cause deterioration of the platelets. A novel procedure has been developed using only short-wave UV light (UVC, 254 nm) that effectively inactivates pathogens in plasma-reduced PCs. The equipment used consists of an irradiation device with a specific mechanism for agitation. Its capacity is one platelet unit (random donor or apheresis) per treatment cycle. Treatment parameters, e.g. UVC intensity, UVC dose, temperature and agitation, are microprocessor-controlled. Platelets are processed in the THERAFLEX twin-bag kit, which comprises a highly UV-transparent polyolefin acetate bag[1] for irradiation and a platelet storage container (Fig.1, 2). We investigated to what extent platelet integrity and storage stability of the treated products were influenced by this new inactivation procedure.

MATERIALS & METHODS

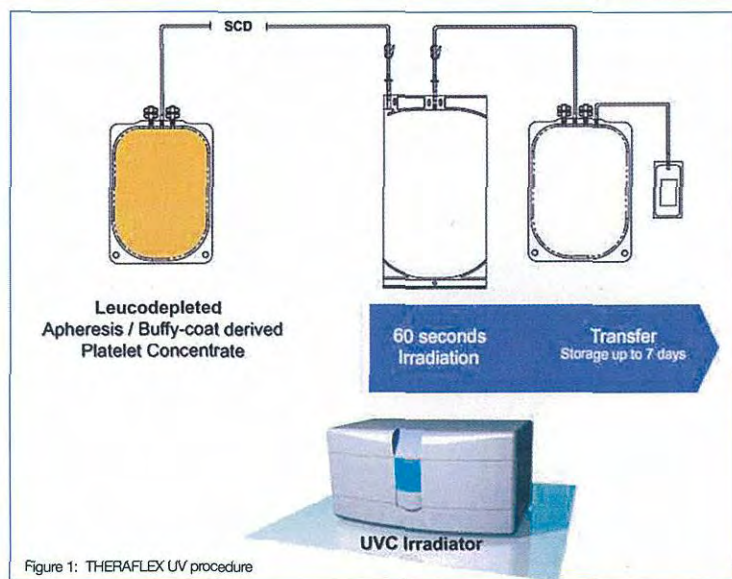

Plasma-reduced PCs were treated with the THERAFLEX UV procedure (Fig. 1) and stored until day 8 after blood donation (day 6 after treatment). The in vitro quality of UVC treated PCs was evaluated in comparison to non-treated control platelets. Control PCs were stored for the same time period. PCs in storage medium SSP+ (MacoPharma) were prepared from pools of 5 buffy coats. The average volume treated was 350 mL. Plasma concentration was approx. 30%. PCs were transferred into irradiation bags (Fig. 2) for UVC treatment. After insertion into the irradiation device (Fig. 3) PCs were treated with UVC light at a dose of 0.4 J/cm² (approx. 60 sec). They were strongly agitated at a frequency of 1.8 Hz during irradiation. The system was microprocessor-controlled. The control unit enables monitoring and recording of relevant treatment parameters like dose, intensity, temperature and irradiation time.



RESULTS

Until day 8 of storage in vitro characteristics were hardly influenced by the THERAFLEX process. HSR reactivity was only slightly reduced whereas collagen induced aggregation was moderately increased. Glucose consumption and lactate formation were found to be marginally higher in the treated PCs. Thus, pH slightly dropped but remained above 7.0 until day 8 after donation. The mean platelet loss due to UVC treatment was 4%. (Tab. 1)

	Pts [x10 ⁹ /mL]	HSR [%]	pH	Spontaneous aggregation [%]	Collagen-ind. aggregation 100 µg/mL [%]	Glucose [mg/dL]	Lactate [mmol/L]
Day 3							
Control	10.2 ± 1.6	68 ± 4	7.13 ± 0.05	11 ± 3	94 ± 3	122 ± 8	7.5 ± 1.0
Treated	9.6 ± 1.3	64 ± 5	7.07 ± 0.07	14 ± 2	89 ± 5	118 ± 6	7.7 ± 0.8
Day 6							
Control	9.9 ± 1.0	66 ± 2	7.24 ± 0.13	12 ± 2	74 ± 9	86 ± 10	10.8 ± 1.0
Treated	9.5 ± 1.3	64 ± 8	7.09 ± 0.06	14 ± 3	81 ± 9	68 ± 10	12.8 ± 1.5
Day 8							
Control	9.4 ± 1.6	68 ± 1	7.29 ± 0.12	10 ± 1	62 ± 7	63 ± 9	12.5 ± 0.9
Treated	9.1 ± 1.3	61 ± 8	7.09 ± 0.05	16 ± 4	69 ± 7	41 ± 8	15.2 ± 1.0

Table 1: Platelet parameters of untreated and treated PCs on day 3, 6 and 8 after blood donation (mean +/- SD; n=4)

CONCLUSIONS

Plasma-reduced PCs were only slightly affected when treated with the THERAFLEX UV system for pathogen inactivation. In vitro parameters and storage stability were well preserved until day 8 after blood donation.

[1] Polyolefineacetate bags for pathogen inactivation and for storage of platelet concentrates, H Mohr, TH Müller, F Tolksdorf, WH Walker, Vox Sang 2004; 87 (Suppl. 3): 70

Funded by Forschungsgemeinschaft der Blutspendedienste des Deutschen Roten Kreuzes e.V. and Maco Pharma.

DEGRADATION OF HUMAN HEPATITIS B VIRUS DNA IN PLATELET CONCENTRATES BY SHORT WAVE ULTRAVIOLET LIGHT AS REVEALED BY REAL-TIME PCR

J. Knüver-Hopf, H. Mohr and T.H. Müller

Blood Center of the German Red Cross Chapters of NSTOB
Institute Springe, Germany

Supported by Forschungsgemeinschaft der Blutspendedienste des Deutschen Roten Kreuzes e.V. & MacoPharma Int.

Conclusion

The present results demonstrate HBV nucleic acid degradation after UVC treatment. This suggests that HBV in platelet concentrates is sensitive to UVC light.

Introduction

Treatment of platelet concentrates (PC) using short wave ultraviolet light (UVC) has been shown to effectively inactivate several pathogens [1]. Inactivation of human hepatitis B virus (HBV) however could not be proven up to now, because there is no infectivity assay available for HBV. The target structures in UVC treatment of viruses is its nucleic acid. Inactivation of viruses therefore might be determined by PCR.

Material and Methods

PC in storage medium SSP+ (MacoPharma, Langen, Germany) containing approx. 30% plasma were prepared from pools of 5 buffy coats. From each PC 120 ml were transferred to ethylvinyl acetate bags from MacoPharma (Langen, Germany). In this study, treatment with UVC light was performed with different doses on a BS10-illumination device (GROEBEL, Ettlingen, Germany). Routinely UVC treatment was done with a dose of 0.4 J/cm². The QIAamp Blood Mini Kit (QIAGEN, Hilden, Germany) was used for isolation of DNA from all samples. For long-range real-time PCR [LR-PCR] the LightCycler was used (ROCHE, Mannheim, Germany). Primers and hybridization probes were synthesized by TIB MOLBIOL (Berlin, Germany). Primers were selected for the nucleotide positions 44 to 2187 of the circular HBV genome.

References

1. Mohr, H.; Gravemann, U.; Bayer, A.; Tolksdorf, F.; Walker, W.H. and Müller, T.H. Sterilization of platelet concentrates by irradiation with short wave ultraviolet light *Vox Sang.* (2007) **93** (Suppl.1) 51
2. Knüver-Hopf, J.; Redecker-Klein, A.; Lambrecht, B. and Mohr, H. Guanine boxes within the genome indicate susceptibility of viruses to photodynamic treatment *Infusionsther. Transfusionsmed.* (1997) **24** 213
3. Knüver-Hopf, J.; Vogt, I. and Mohr, H. The influence of photodynamic treatment on the genome and the infectivity of parvovirus B19 *Transfusion clinique et biologique* (2001) **8** (Suppl.1) 99
4. Knüver-Hopf, J.; Mohr, H. and Müller, T.H. Photodynamic inactivation of human hepatitis B virus in plasma as revealed by long-range PCR *Vox Sang.* (2005) **89**(Suppl.1) 10
5. Knüver-Hopf, J.; Gravemann, U.; Mohr, H., and Müller, T.H. Photodynamic inactivation of human hepatitis B virus in plasma-reduced platelet concentrates as revealed by long-range real-time PCR *Transfusion Medicine* (2006) **33** (Suppl.1) 63

Results and Discussion

From previous investigations it is known that PCR inhibition cannot be shown by a short-range HBV real-time PCR [2]. This is probably due to the short genome region analysed. This finding is in agreement with previous PCR studies with HIV-1 and parvovirus B19. In those studies we found a correlation between the analysed viral genome region and inhibition of PCR in virus-infected samples after photodynamic treatment [3-5]. In the present study the effect of UVC treatment on HBV-DNA was evaluated by the use of LR-PCR. An increased amplicon size of 1090 base pairs was a sufficient target to demonstrate the effect of UVC treatment. As seen in figure 1, the fluorescence curves of treated samples shifted towards higher cycle number values compared to untreated samples. As shown in figure 2, the PCR signals were lowered from 100% to 2% after treatment with 0.4 J/cm² of UVC, i.e. from approx. 10x10⁷/ml genome copies to 10x10⁵/ml.

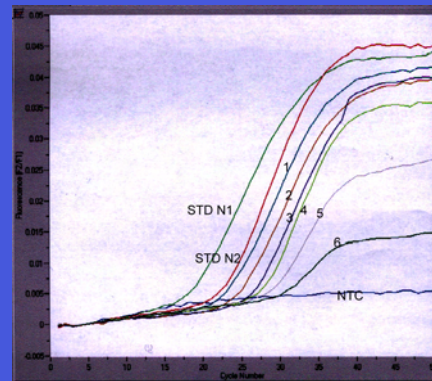


Figure 1: Amplification plot of LR-PCR before and after pathogen inactivation procedure with UVC of HBV in platelet concentrates **1)** untreated HBV sample; **2-6)** UVC- treated HBV sample; 0.1, 0.3, 0.4, 0.5 and 0.6 J/cm² **STD N1 and N2)** calibration standards; **NTC)** no template control

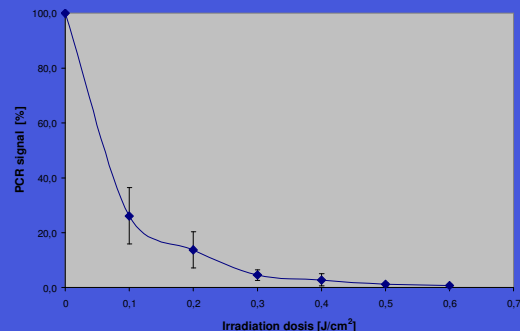


Figure 2: Kinetics of nucleic acid degradation of HBV in PC after UVC treatment detected by LR-PCR
N=6; +/-SD

THERAFLEX UV PLATELETS: NOTHING BUT UVC LIGHT AND STRONG AGITATION

H. Mohr¹, U. Gravemann¹, F. Tolksdorf², W.H. Walker², T.H. Müller¹

Purpose

Blood donations may not only be contaminated with viruses, e.g. HBV, HCV or HIV. In addition, they may contain bacteria. This is especially crucial for platelet concentrates (PCs), because they have to be stored at room temperature, at which bacteria can multiply to high levels [1-2].

Short-wave ultraviolet light (UVC, wavelength range: 200-280 nm) is germicidal, but low UV-permeability hampers its use for sterilizing PCs. A simple method was developed which overcomes this limitation.

Materials and Methods

Plasma-reduced PCs in storage medium SSP+ (volume approx. 350 mL, platelet concentration approx. 10⁹/mL, plasma content 30-35%) were prepared from pools of 5 buffy coats [3]. PC volume was approx. 350 mL. The PCs were spiked with approx. 10²-10⁶ CFU/mL of different bacteria species or up to 10⁷ TCID₅₀/mL of lipid-enveloped or nonenveloped viruses. Other PCs were spiked with 5x10⁶/mL peripheral blood mononuclear cells (PBMC). The PCs were filled into UV-transparent plastic bags and irradiated on a device (Fig.1), equipped with mercury vapour tubes emitting monochromatic UVC-light (wavelength: 254 nm). The device was equipped with an orbital agitator. Irradiation was from both sides of the bags. UVC doses applied were up to 0.6 J/cm² (approx. 90 sec). During treatment the PCs were strongly agitated. Bacteria or virus titers, PBMC viability and platelet parameters were determined before and after irradiation. Each experiment was repeated 3-6 times. Results are depicted as mean ± SD.

Results

Pathogen inactivation was enormously enhanced when the PCs were loosely placed on a quartz plate located between the two layers of UVC tubes of the irradiation device and, in addition, strongly agitated during irradiation (Fig. 2).

UVC-light at 0.3-0.4 J/cm² (irradiation time: approx. 1 min) reduced the titers of all bacteria tested by approx. 5-6 log₁₀ steps. PCs spiked with approx. 100 CFU/ml of bacteria were reproducibly sterilized (Tab.1). In one experiment with *B. cereus* the PC was sterile after 3 but unsterile after 6 days storage. This was probably due to spores of *B. cereus* that are more resistant to UVC than vegetative bacteria.

UVC sensitivity of the viruses tested was not so uniform (Table 1): The small single stranded RNA viruses VSV, Sindbis and WNV were completely inactivated at approx. 0.3-0.4 J/cm². Remarkably HIV-1 (also a small single-stranded RNA virus) was only moderately inactivated at UVC doses up to 0.6 J/cm².

The small nonenveloped DNA viruses PPV and EMCV proved to be very sensitive. Complete inactivation was achieved at 0.4-0.5 J/cm².

With the exception of HIV-1, SHV-1 was more resistant than the other viruses tested. This confirms that in general large double stranded DNA viruses are not as susceptible to UVC as smaller single stranded DNA or RNA viruses.

PBMC proved to be extremely sensitive to UVC irradiation: Complete inactivation was found at less than 0.1 J/cm² (Fig. 3)

PC properties remained almost unchanged at doses up to 0.6 J/cm². The storage stability of the treated PCs for up to 6 days after treatment (8 days after blood donation) was maintained (Table 2)

Conclusions

Irradiation with UVC under strong agitation may be used to sterilize platelet concentrates at a light dose that is not harmful to the products. The UVC dose required is 0.4 J/cm². Irradiation time is not more than approx. 1 min.

Parameter	Day 1 after irradiation				Day 6 after irradiation			
	Control	UVC dose (J/cm ²)			Control	UVC dose (J/cm ²)		
		0.4	0.5	0.6		0.4	0.5	0.6
Pts [x10 ⁹ /mL]	10.8 ± 0.6	10.2 ± 0.6	9.8 ± 0.6	9.1 ± 0.9	10.1 ± 0.8	9.8 ± 0.6	9.3 ± 0.8	9.3 ± 0.9
pH	7.10 ± 0.04	7.04 ± 0.05	7.09 ± 0.05	7.05 ± 0.04	7.27 ± 0.15	7.09 ± 0.06	7.11 ± 0.10	6.98 ± 0.07
Lactate [mmol/L]	7.7 ± 1.0	8.0 ± 0.5	7.7 ± 0.5	8.0 ± 0.7	12.7 ± 1.0	14.9 ± 1.0	14.6 ± 1.4	16.7 ± 1.4
Glucose [mg/dL]	122 ± 9	117 ± 7	117 ± 6	115 ± 7	62 ± 11	43 ± 8	44 ± 11	29 ± 10
Swirling	ok	ok	ok	ok	ok	ok	ok	ok
HSR [%]	69 ± 5	66 ± 2	61 ± 6	62 ± 4	68 ± 2	65 ± 2	62 ± 3	56 ± 5
Collagen-induced aggregation [%]	95 ± 4	90 ± 5	88 ± 3	87 ± 2	62 ± 9	69 ± 8	67 ± 2	69 ± 5
CD62 [%]	36 ± 1	46 ± 3	47 ± 2	49 ± 1	29 ± 1	45 ± 8	50 ± 10	57 ± 8
Annexin V [%]	5 ± 1	6 ± 3	7 ± 4	7 ± 4	9 ± 5	8 ± 2	10 ± 2	12 ± 3

Tab. 3: Treatment of PCs with different UVC doses. Influence on platelet parameters and on storage stability. n=6, mean + SD




Fig. 1 : Irradiation device for UVC treatment of PCs





Fig. 2 : Inactivation of *St. epidermidis* in PC aliquots (110 or 280 mL) by irradiation with UV light: fixed vs. loosely placed irradiation bags (a); dependence of bacteria inactivation in loosely placed irradiation bags on the agitation speed (b). n=3, mean ± SD

Bacteria species	Characteristics	Gram stain	Number pf experiments	Spike (CFU/mL)	Bact/Alert result*	Remark
<i>B. cereus</i>	fac. anaerobic	pos	12	100-140	11 sterile 1 unsterile**	Spore former
<i>E. coli</i>	aerobic	neg	12	36-65	12 sterile	
<i>K. pneumoniae</i>	fac. anaerobic	neg	12	85-140	12 sterile	
<i>P. acnes</i>	anaerobic	neg	12	61-100	12 sterile	
<i>S. aureus</i>	fac. anaerobic	pos	22	60-110	22 sterile	
<i>S. epidermidis</i>	fac. anaerobic	pos	22	74-210	22 sterile	
<i>Str. pyogenes</i>	fac. anaerobic	pos	12	118-194	12 sterile	

*: Samples (2x10 mL each) were drawn after 3 and 6 days at 22°C
**: sterile after 3 days storage

Tab 1: Sterilization of PCs spiked with different bacteria species by irradiation with UVC (0.4 J/cm²)

Virus	Genome	Lipid Envelope	Model virus for	Log ₁₀ reduction factor
Vesicular stomatitis (VSV)	ss ⁺ RNA	X	-	≥ 6.41
Sindbis (Sindbis)	ss RNA	X	-	5.55
West Nile (WNV)	ss RNA	X	HCV	5.24
Human immunodeficiency (HIV-1)	ss RNA	X	-	1.36
Suid Herpes (SHV-1)	ds ⁺ DNA	X	HBV/CMV	3.57
Porcine Parvo (PPV)	ss DNA	-	Parvo B 19	≥ 6.42
Encephalomyocarditis (EMCV)	ss DNA	-	HAV	5.73

Tab 2: Inactivation factors of viruses by irradiation with UVC (0.4 J/cm²)

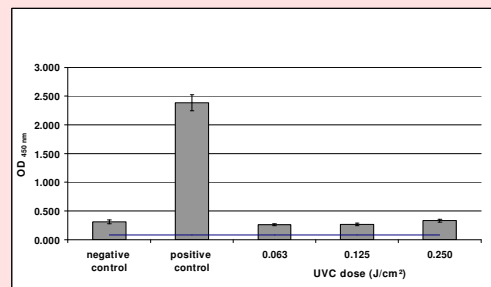


Fig. 3: Inactivation of T-lymphocytes in platelet concentrates by irradiation with UVC. Viability was assayed by mixed lymphocyte culture.

References

- Wagner SJ. Transfusion-transmitted bacterial infection: risks, sources and interventions. Vox Sang 2004;86(3):157-63.
- Mohr H, Bayer A, Gravemann U, Muller TH. Elimination and multiplication of bacteria during preparation and storage of buffy coat-derived platelet concentrates. Transfusion 2006;46(6):949-55.
- Eriksson L, Shanwell A, Gulliksson H, et al. Platelet concentrates in an additive solution prepared from pooled buffy coats. In vivo studies. Vox Sang 1993;64(3):133-8

¹ + Blood Center of the German Red Cross Chapters of NSTOB, Springe, Germany

² MacoPharma Int., Langen, Germany

Supported by Forschungsgemeinschaft der Blutspendedienste des Deutschen Roten Kreuzes e.V.

INACTIVATION OF SMALL NON-ENVELOPED VIRUSES IN PLASMA REDUCED PLATELET CONCENTRATES BY IRRADIATION WITH SHORT-WAVE ULTRAVIOLET LIGHT

H. Mohr¹, U. Gravemann¹, J. Knüver-Hopf¹, F. Tolksdorf², W.H. Walker², T.H. Müller¹

Aim

To investigate if small nonenveloped viruses in plasma reduced platelet concentrates are sensitive to irradiation with UVC light.

Introduction

Small nonenveloped viruses (e.g. parvovirus B19 and hepatitis A virus) are more resistant than lipid-enveloped viruses to most pathogen reduction procedures used for plasma or for cellular blood products (1-3). We have developed a procedure to decontaminate platelet concentrates (PCs) by irradiation with monochromatic short-wave ultraviolet light (wavelength: 254 nm). It is essential that the products are not fixed and at the same time strongly agitated during treatment (Fig. 1 and 2). We found that the procedure inactivates bacteria and lipid enveloped viruses. As the present data indicate, small nonenveloped viruses are also inactivated.

Materials and Methods

The virological investigations were conducted at NewLab BioQuality, Cologne, Germany. They were carried out according to CPMP/BWP guidelines 268/95 ("Note for guidance on virus validation studies") and 269/95 ("Note for guidance on plasma derived medicinal products"). The PCR investigations were performed in the own laboratory. Plasma-reduced PCs (platelet concentration approx. 10⁹/mL, plasma content: approx. 30 %) were prepared from pools of 5 buffy coats. The storage medium used was SSP⁺ (MacoPharma). PCs (volume approx. 350 mL) in UV transparent polyolefine acetate bags (dimensions: 19x38 cm) were spiked with approx. 10⁷ up to 10⁸ TCID₅₀/mL of porcine parvovirus (PPV, strain ATCC CRL-6489 (NADL-2), a model for parvovirus B19) or echinocystidiosis virus (EMCV, strain ATCC VR 129-B, a model for hepatitis A virus). The thickness of the PC layer was approx. 4-5 mm. Irradiation with UVC light was from both sides of the bags. The UVC dose applied was up to 0.6 J/cm² (irradiation time per 0.1 J/cm² was approx 15 sec). The PC-samples were loosely placed on a quartz plate located in the middle between two layers of mercury vapor tubes emitting monochromatic UVC light (wavelength: 254 nm). During irradiation they were intensively agitated using an orbital agitator. Agitation speed was approx. 100 rpm. Before and after irradiation virus titers (expressed as log₁₀ of tissue culture infectious doses (log₁₀TCID₅₀)) were determined. The influence of UVC on the DNA of parvovirus B19 was investigated by long-range RT-PCR, using a LightCycler from Roche, Mannheim, Germany. The primer pair used spanned a region of 1028 bases (approx. one fifth of the genome of the virus). In these experiments PC aliquots of 110 mL were treated; dimensions of the irradiation bags were 12.5x14.5 cm.

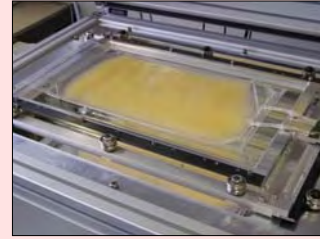


Fig. 1 and 2: Irradiation device for UVC treatment of PCs

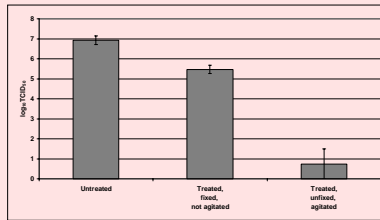


Fig. 2: Inactivation of vesicular stomatitis virus by irradiation with UVC (n=3). Comparison of two treatment modes: Fixed bags (changed between 2 quartz plates) vs. unfixed bags (loosely put on a quartz plate), both with agitation (100 rpm)

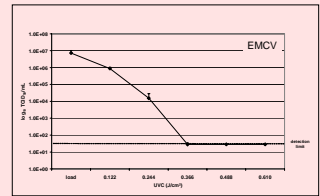
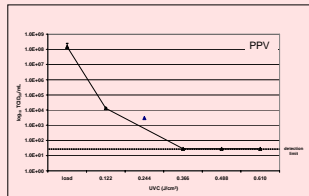


Fig. 3: Inactivation kinetics of PPV and EMCV in plasma-reduced PCs irradiated with UVC. (n=2).

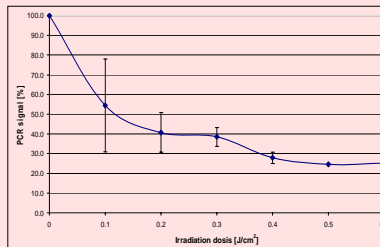


Fig. 4: Degradation of the DNA of parvovirus B19 spiked into plasma-reduced PCs by irradiation with UVC. (n=3, mean ± SD).

Results

PPV as well as EMCV in plasma-reduced PCs were rapidly inactivated by irradiation with UVC light: no infective virus was detectable at doses higher than 0.366 J/cm² (Fig. 3). The log₁₀ reduction factors determined exceeded 6.4 and 5.5, respectively. The PCR investigations revealed that the genome of parvovirus B19 was degraded by UVC treatment: at light doses between 0.4 and 0.6 J/cm² the PCR signal was reduced by approx. 75 % (Fig. 4). It remains to be established if this is indicative of complete inactivation of that virus. At UVC doses up to 0.6 J/cm² platelet functions were only moderately influenced, and the storage stability of the treated products for up to 6 days after treatment (8 days after blood donation) was maintained (Table 1).

Conclusions

Irradiation with UVC light under strong agitation is a unique procedure to inactivate small nonenveloped viruses in PCs at conditions at which platelet functions and the storage stability of the PCs are not impaired.

References

- Welch J, Bienek C, Gomperts E, Simmonds P. Resistance of porcine circovirus and chicken anemia virus to virus inactivation procedures used for blood products. *Transfusion* 2006;46(11):1951-8.
- Lin L, Hanson CV, Alter HJ, et al. Inactivation of viruses in platelet concentrates by photochemical treatment with amotosalen and long-wavelength ultraviolet light. *Transfusion* 2005;45(4):380-90.
- Mohr H, Lambrecht B, Seiz A. Photodynamic virus inactivation of blood components. *Immunol Invest* 1995;24(1-2):73-85.

Parameter	Day 1 after irradiation				Day 4 after irradiation				Day 6 after irradiation			
	Control	UVC dose (J/cm ²)			Control	UVC dose (J/cm ²)			Control	UVC dose (J/cm ²)		
		0.4	0.5	0.6		0.4	0.5	0.6		0.4	0.5	0.6
Plt-concentration (x10 ⁹ /L)	10.8 ± 0.6	10.2 ± 0.6	9.8 ± 0.6	9.1 ± 0.9	10.3 ± 0.8	10.1 ± 0.8	9.6 ± 0.8	9.5 ± 0.9	10.1 ± 0.8	9.8 ± 0.6	9.3 ± 0.8	9.3 ± 0.9
pH	7.10 ± 0.04	7.04 ± 0.05	7.09 ± 0.05	7.05 ± 0.04	7.21 ± 0.14	7.06 ± 0.04	7.10 ± 0.06	7.06 ± 0.20	7.27 ± 0.15	7.09 ± 0.06	7.11 ± 0.10	6.98 ± 0.07
Lactate (mmol/L)	7.7 ± 1.0	8.0 ± 0.5	7.7 ± 0.5	8.0 ± 0.7	10.7 ± 1.2	12.3 ± 1.3	11.7 ± 1.3	13.8 ± 2.0	12.7 ± 1.0	14.9 ± 1.0	14.6 ± 1.4	16.7 ± 1.4
Glucose (mg/dL)	122 ± 9	117 ± 7	117 ± 6	115 ± 7	86 ± 12	70 ± 10	75 ± 10	58 ± 15	62 ± 11	43 ± 8	44 ± 11	29 ± 10
Swirling	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok
Hypotonic shock response [%]	69 ± 5	66 ± 2	61 ± 6	62 ± 4	66 ± 3	67 ± 4	65 ± 3	61 ± 3	68 ± 2	65 ± 2	62 ± 3	56 ± 5
Spontaneous aggregation [%]	11 ± 2	14 ± 2	18 ± 3	18 ± 3	12 ± 2	15 ± 2	15 ± 1	17 ± 6	10 ± 2	16 ± 4	13 ± 2	14 ± 1
Collagen-induced aggregation [%] 100 µg/mL	95 ± 4	90 ± 5	88 ± 3	87 ± 2	77 ± 9	83 ± 10	80 ± 6	83 ± 5	62 ± 9	69 ± 8	67 ± 2	69 ± 5
Collagen-induced aggregation [%] 20 µg/mL	54 ± 13	77 ± 8	78 ± 6	74 ± 8	15 ± 7	35 ± 12	33 ± 9	39 ± 8	9 ± 1	16 ± 4	19 ± 1	22 ± 2
CD62 [V]	36 ± 1	46 ± 3	47 ± 2	49 ± 1	27 ± 3	36 ± 5	42 ± 6	48 ± 5	29 ± 1	45 ± 8	50 ± 10	57 ± 8
Annexin V [%]	5 ± 1	6 ± 3	7 ± 4	7 ± 4	6 ± 3	10 ± 5	9 ± 2	9 ± 2	9 ± 5	8 ± 2	10 ± 2	12 ± 3

Tab. 1: Irradiation of PCs with different UVC doses. Influence on platelet parameters and on storage stability. (n= 6, mean ± SD).

¹ Blood Center of the German Red Cross Chapters of NSTOB, Springe, Germany

² MacoPharma Int., Langen, Germany

Supported by Forschungsgemeinschaft der Blutspendedienste des Deutschen Roten Kreuzes e.V.